NOTICE: This document contains references to Varian. Please note that Varian, Inc. is now part of Agilent Technologies. For more information, go to **www.agilent.com/chem.**

Agilent Technologies

User Manual

External sample filter for Micro-GC

Installation

The External sample filter (Cat.no. CP736729) is recommmended as a pre-filter for the Varian Micro-GC.

The figure below shows the components of the filter and how it is installed between the front panel of the Micro-GC and the sample input line.

Unheated Injector Systems

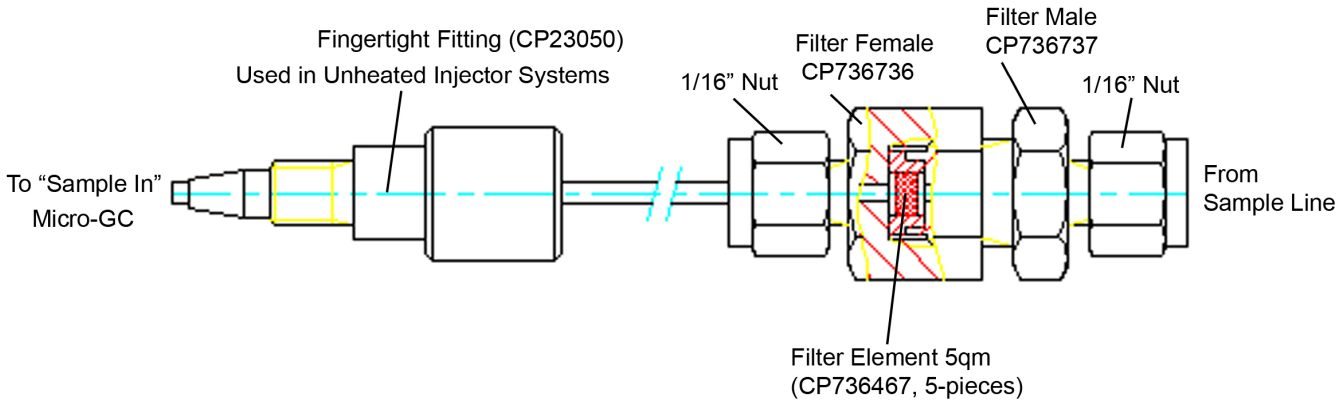

Heated Injector Systems

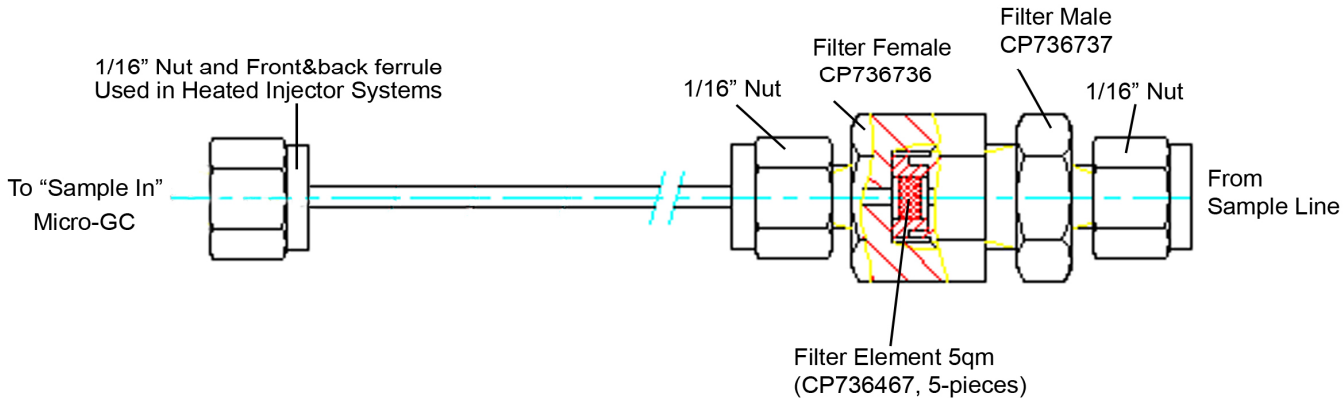

Varian, Inc. All Rights Reserved
Printed in the Netherlands CP505260 Rev: 2 Nov 2004